


MEA60-4Well-Pt, MEA60-4Well-PtBlack

Channel numbers mentioned correspond to the amplifier pin numbers of the MCS MEA-System.

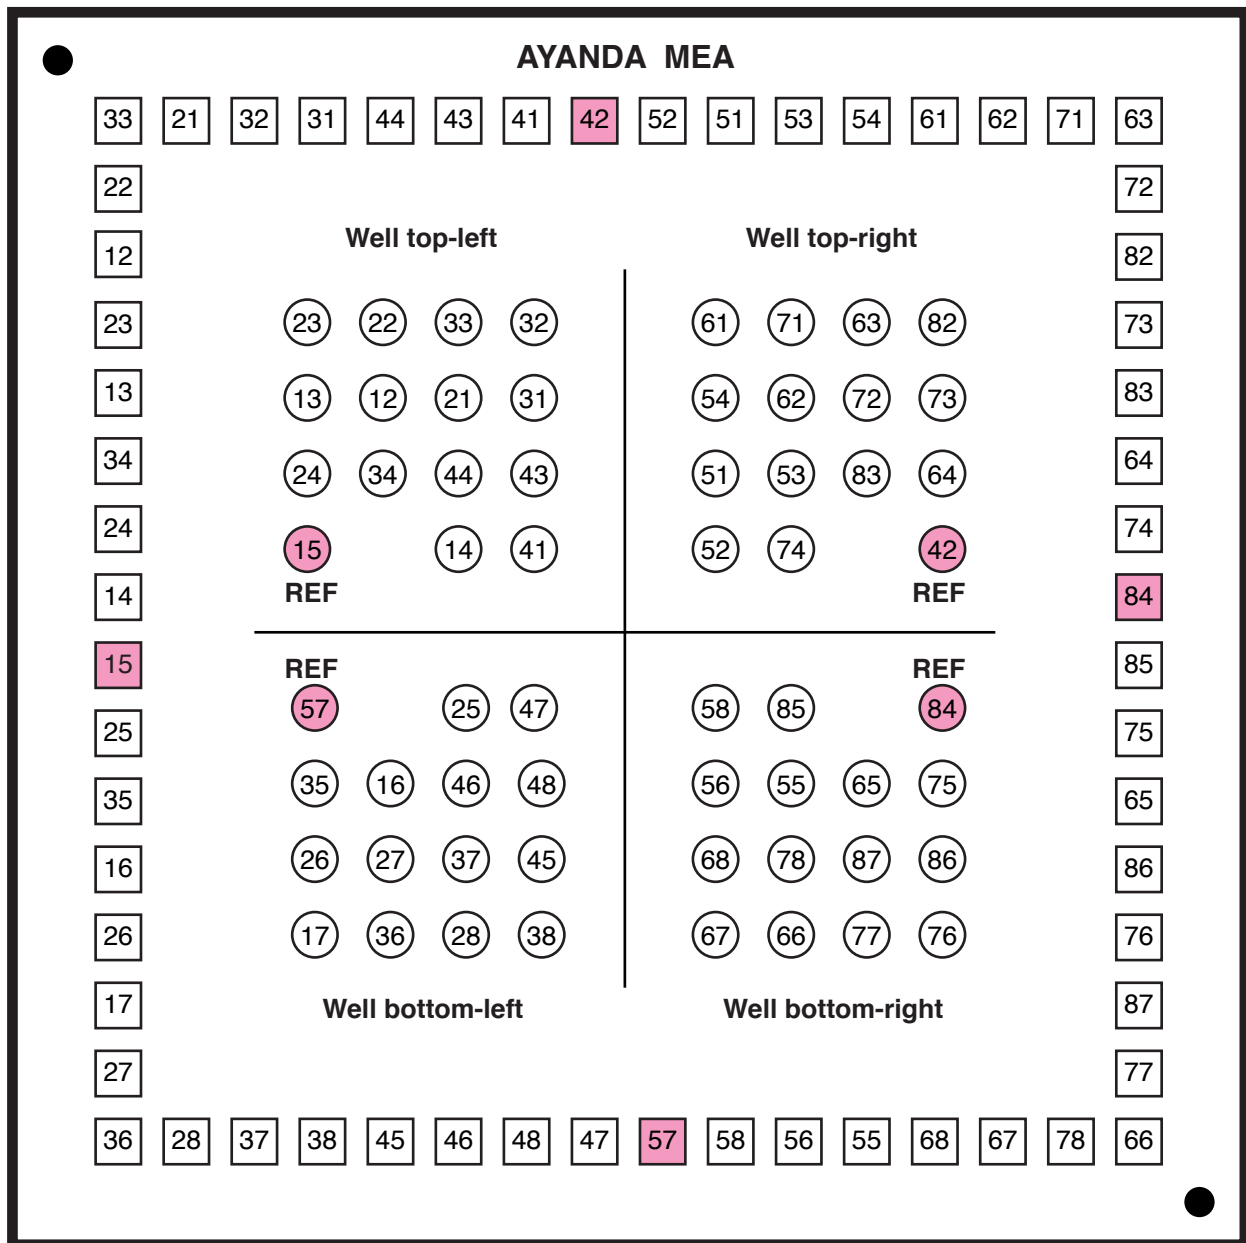

The numbering of the MEA electrodes as shown correspond to the effective electrode locations within the MEA60-4well biochip.

The electrodes number 15, 42, 57 and 84 correspond to independent large internal reference electrode, one in each well, to be connected to the MEA-system reference.

The corresponding MC_Rack mapfile to be used during experiments is named "MEA60_4Well.cmp".